



HEALCERION

Image Gallery

SONON

Smart Healthcare for all

Healcerion Co., Ltd.

Address: 804ho, 38-21, Digital-ro 31-gil,
Guro-Gu, Seoul, 08376 Korea
www.healcerion.com Tel: +82.70.7569.6326,
E-mail: info@healcerion.com
© 2016 Copyright. All Rights Reserved.


General image

Liver

HC 300c_new
HEALCERION 300c_new

96%

R

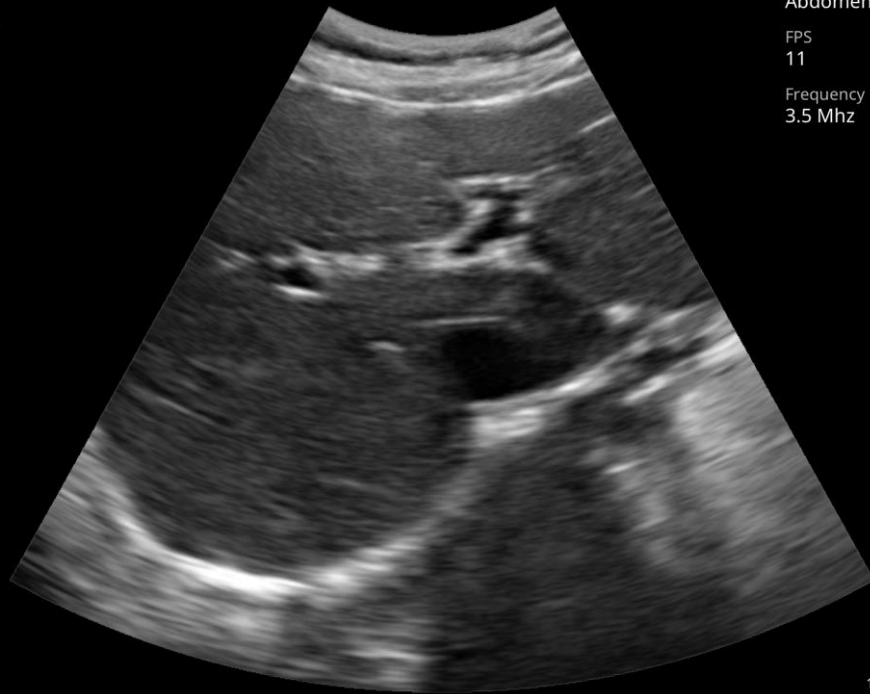

2017/11/03 02:32:46 오후
HC | Unknown
MI:0.48 / TIB:0.20

HC
HEALCERION

20170108


Preset
Abdomen
FPS
11
Frequency
3.5 Mhz

R

17 cm

01/08/2017 10:42:07 오후
Healcerion | Erika
MI:0.48 / TIB:0.20

Preset
Abdomen
FPS
0
Frequency
3.5 Mhz

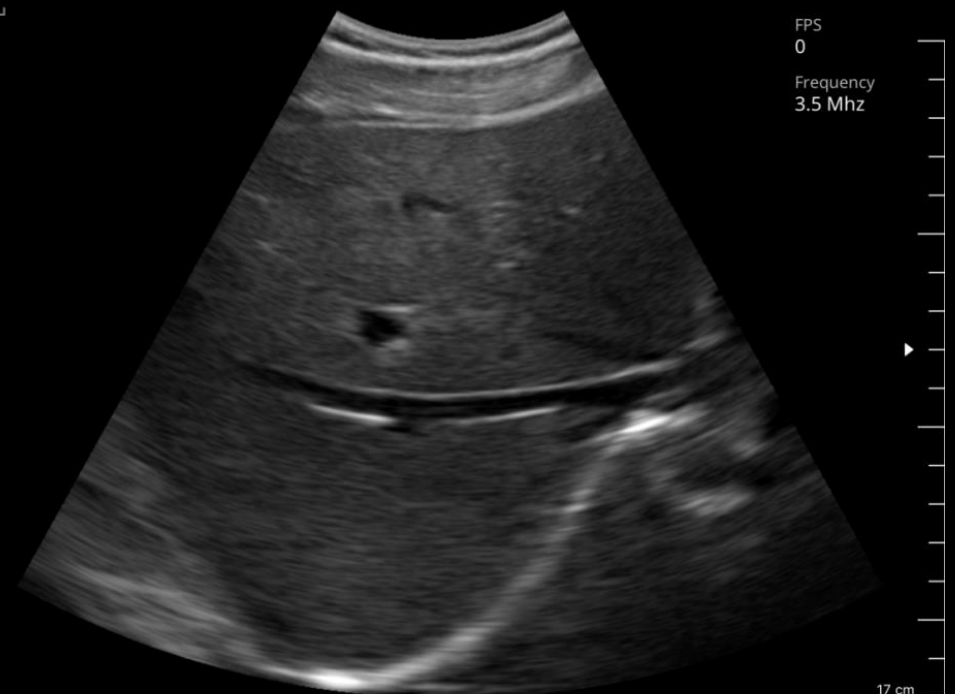


17 cm

Liver



Kidney/Pancreas

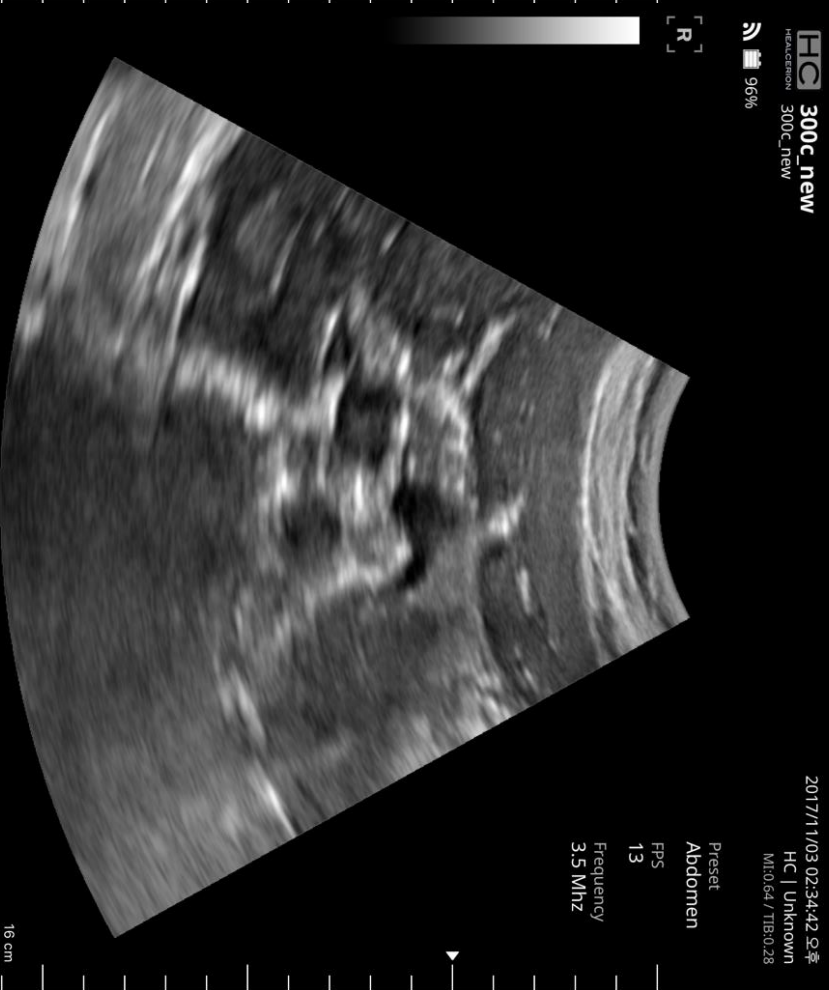

Thyroid



HEALCATION

clinicalimage

1


10/19/2017 14:29:11

q | -

MID.73 / THEO.28

100%

R

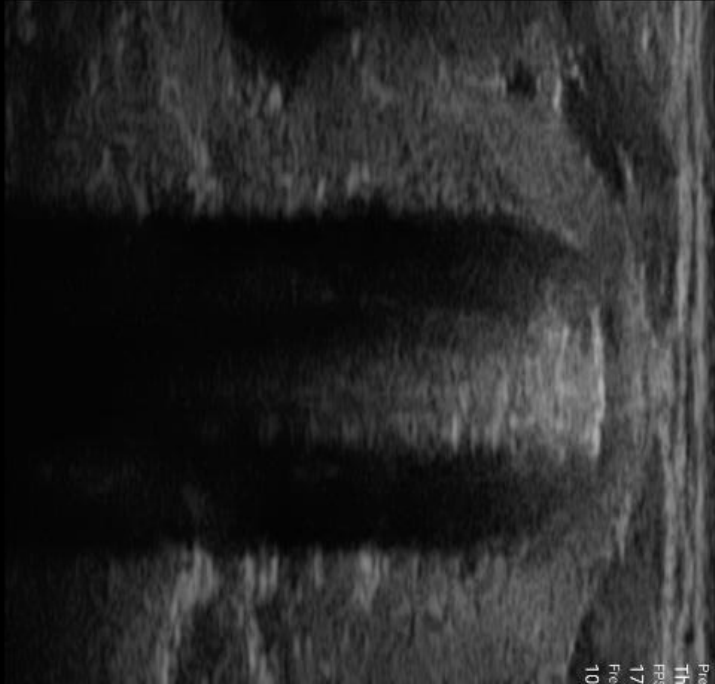

Preset
Thyroid
FPS
17
Frequency
10MHz



HEALCATION

clinicalimage

1

10/19/2017 14:30:52

q | -

MID.73 / THEO.28

100%



R



Preset
Thyroid
FPS
17
Frequency
10MHz



Thyroid

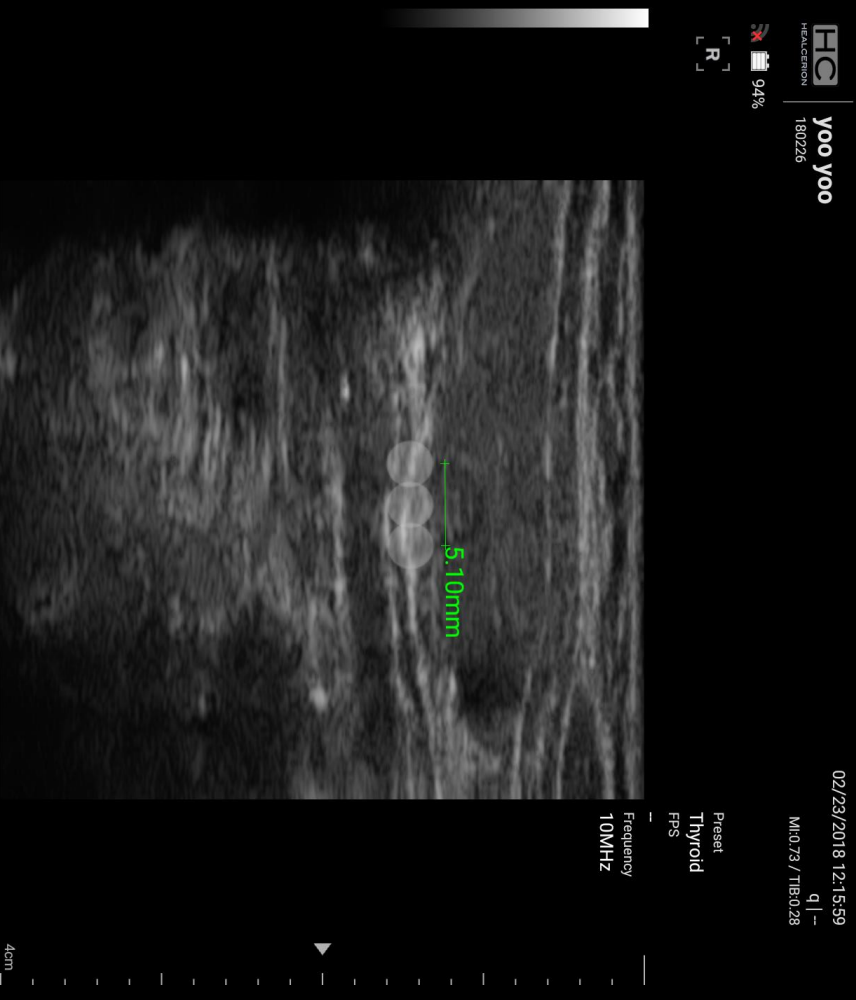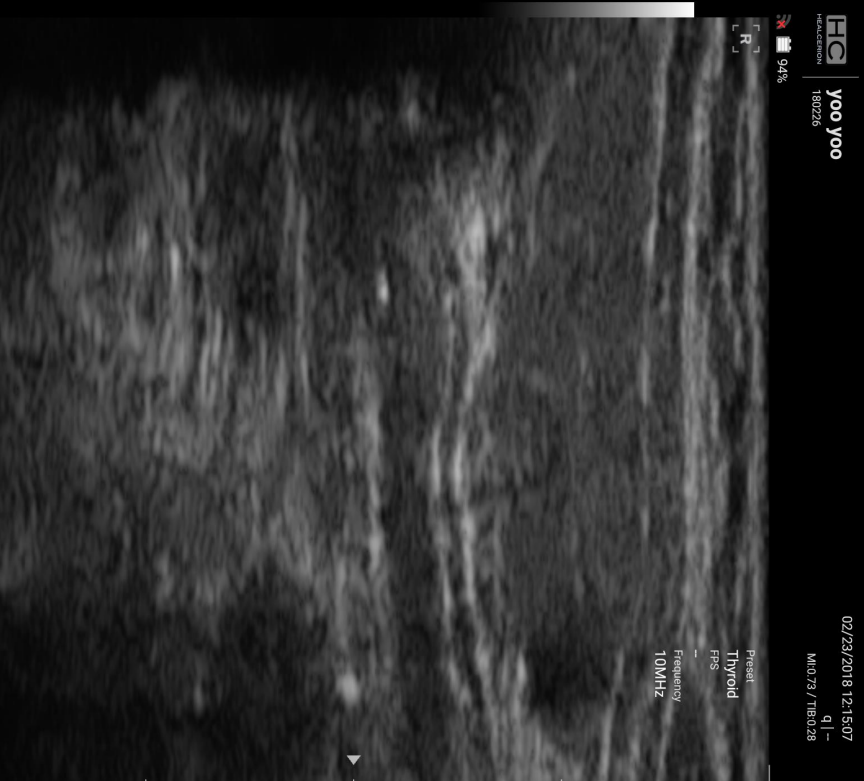


Thyroid benign nodule

Breast



20170108

[R]

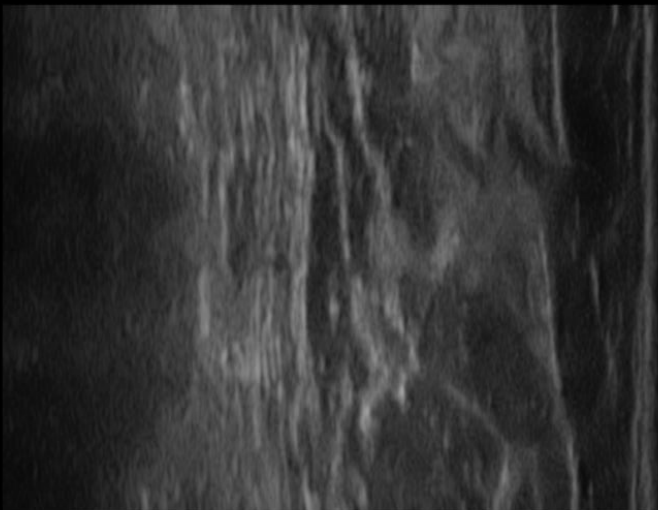

01/09/2017 12:49:32 오전
Healcerion | Erika
MI:0.82 / TIB:0.33

Preset
Breast


FPS
0

Frequency
10 Mhz

[R]



20170108

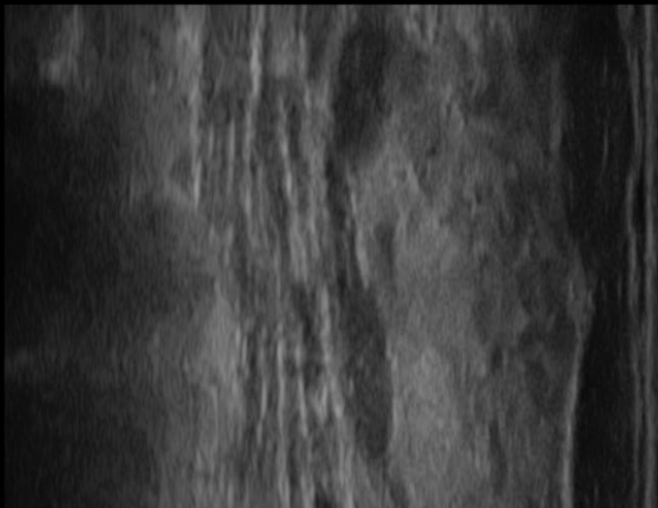


01/09/2017 12:50:08 오전
Healcerion | Erika
MI:0.82 / TIB:0.33

Preset
Breast

FPS
0

Frequency
10 Mhz

[R]



Breast



HEALCERION

20170108

01/09/2017 12:49:42 오전

Healcerion | Erika

MI0082 / TIB0033



HEALCERION


20170108

01/09/2017 12:49:13 오전

Healcerion | Erika

MI0082 / TIB0033

[R]

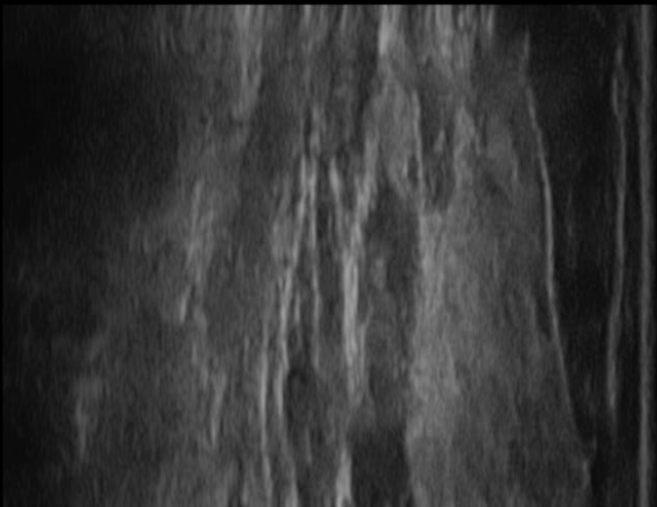

[R]




Preset
Breast

FPS

0

Frequency
10 Mhz

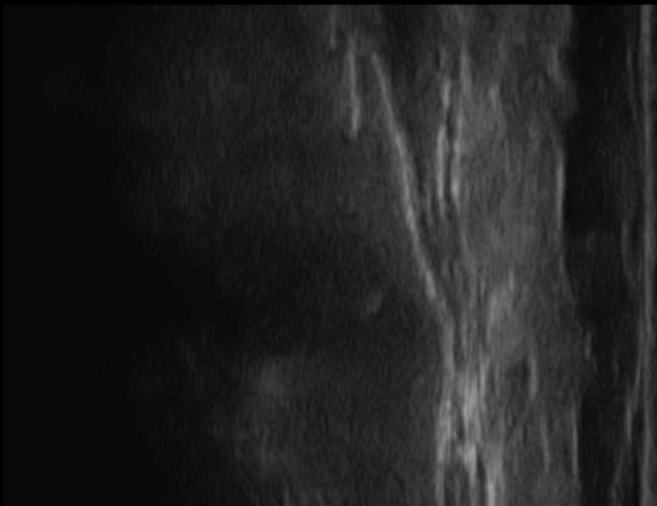

Preset
Breast

FPS

0

Frequency
10 Mhz



OB Gyn

Obstetric



Face



Foot

Obstetric





Abdomen



Femur

Vascular

Carotid

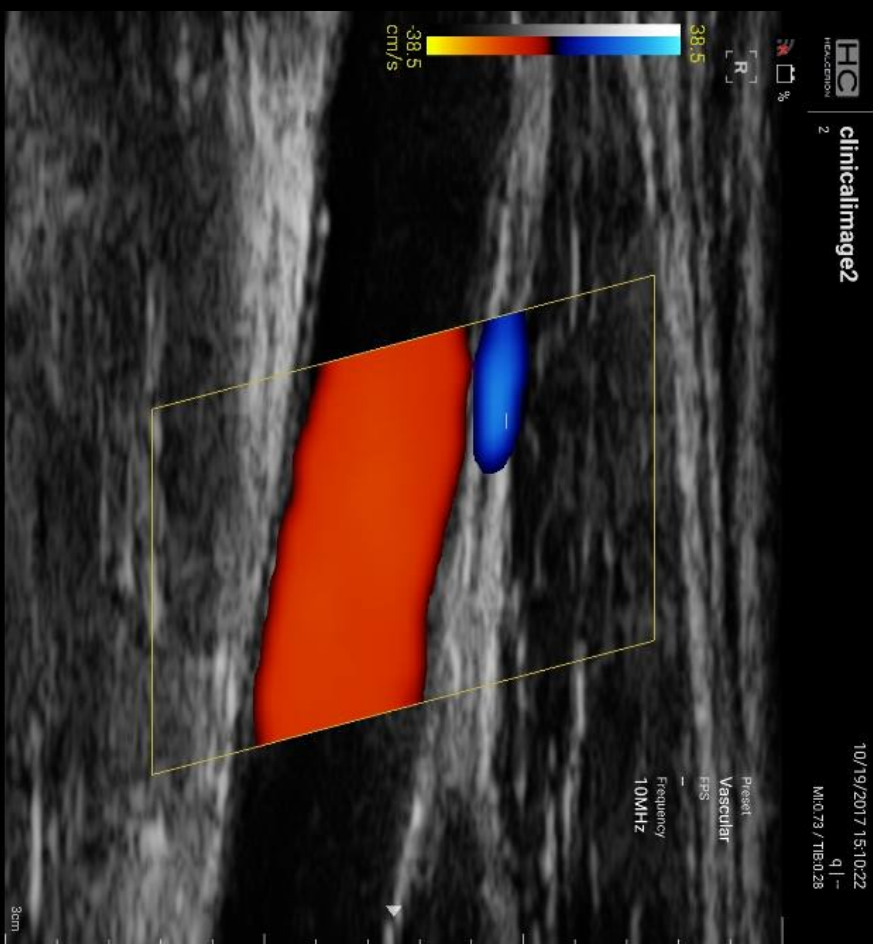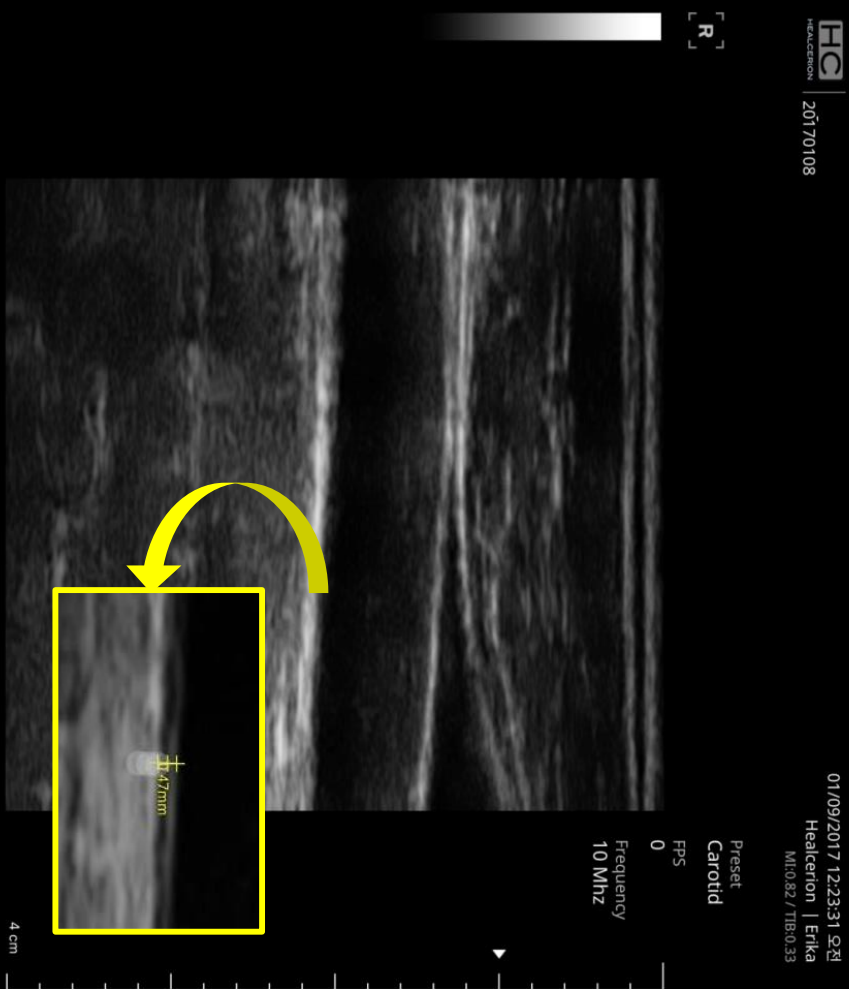


Femoral nerve & artery

HC
HEALCERION | 20170108

01/09/2017 12:46:25 오전
Healcerion | Erika
MI0.82 / TIB0.33


HC
HEALCERION | 20170108

[R]

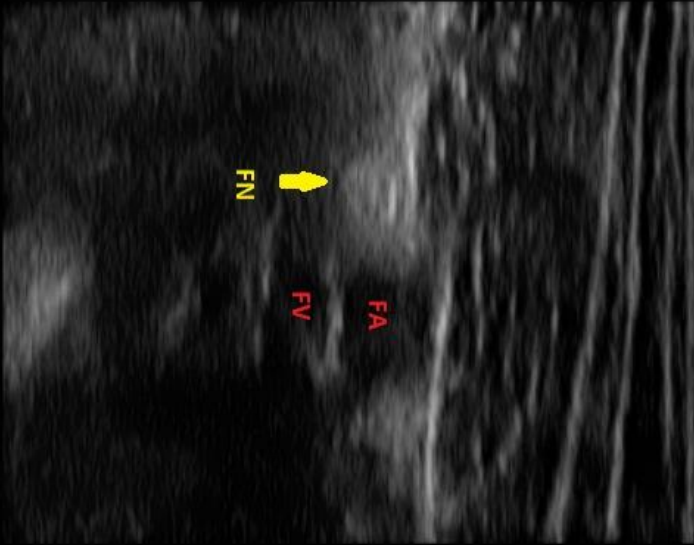

Preset
Vascular


[R]

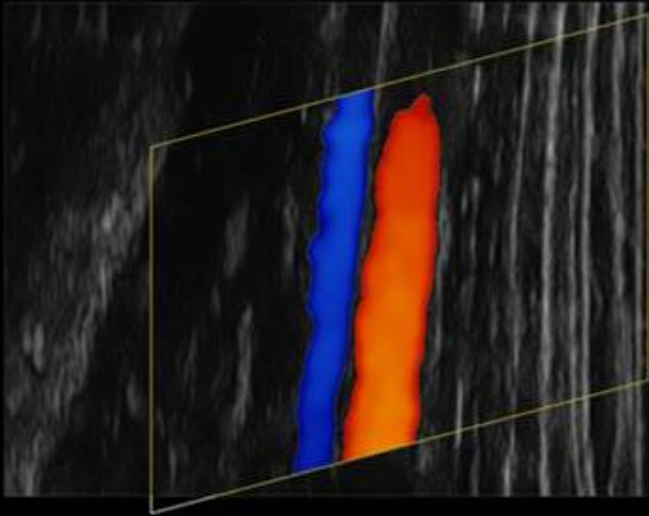

Preset
Vascular

FPS

0
Frequency
10 Mhz



01/09/2017 12:46:25 오전
Healcerion | Erika
MI0.82 / TIB0.33

Musculoskeletal




clinicalimage

10/19/2017 14:40:23

MI0.73 / TIBU.28

99%

[R]

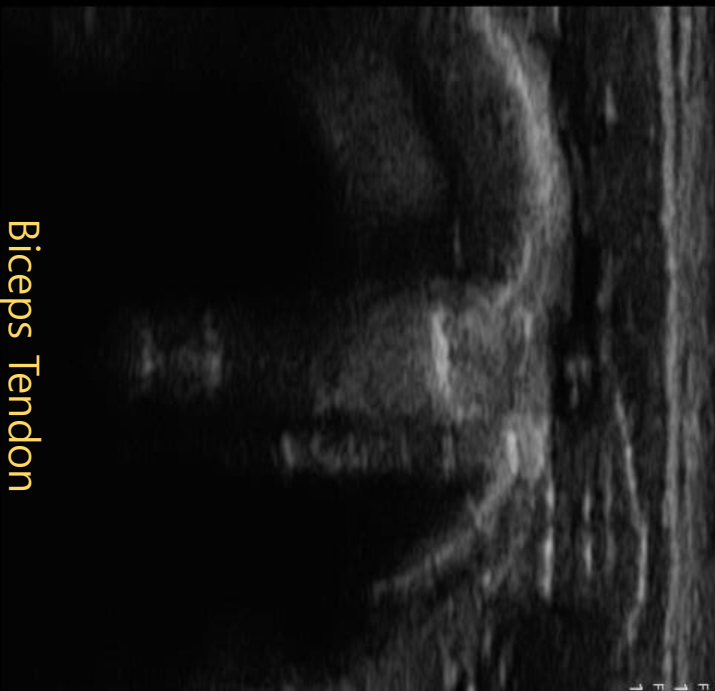

Biceps Tendon

Preset
MSK

FPS

18

Frequency
10MHz



4cm




clinicalimage

10/19/2017 14:44:23

MI0.73 / TIBU.28

98%

[R]

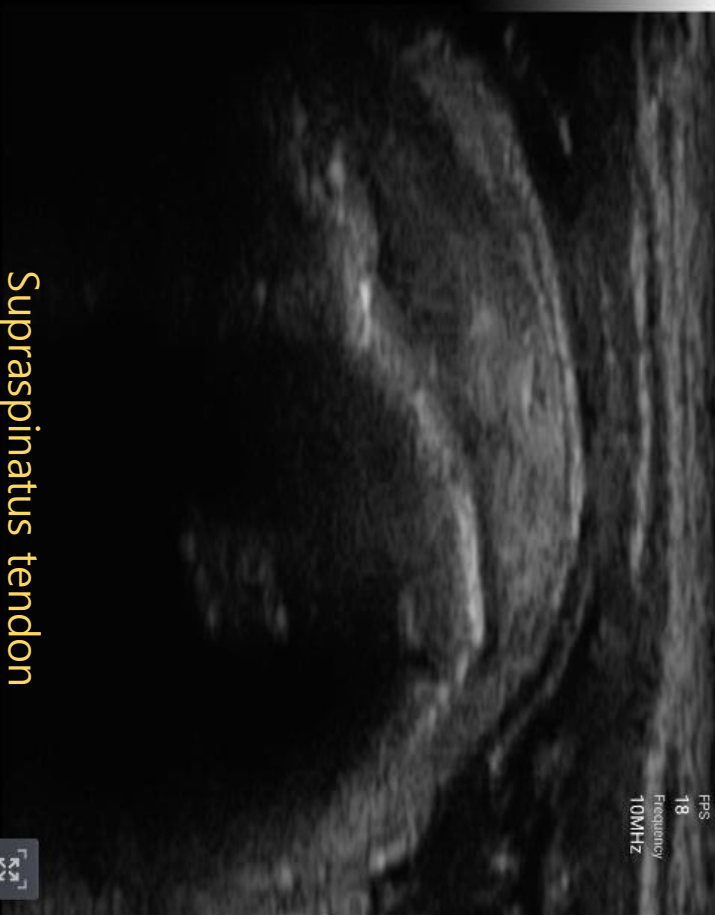

Supraspinatus tendon

Preset
MSK

FPS


18

Frequency
10MHz



3cm

MSK

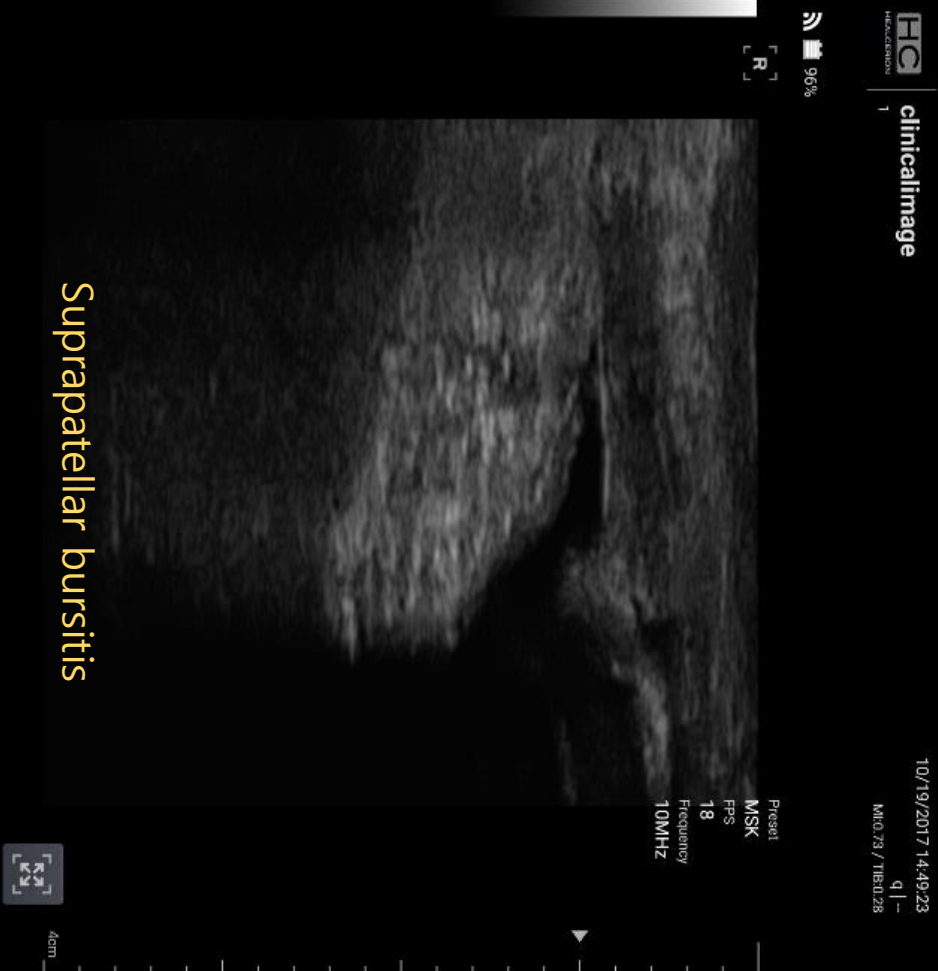

MSK



clinicalimage2

10/19/2017 15:17:05

q | -
MIQ.73 / TIBD.28

85%

「R」

Preset
MSK
FPS
18
Frequency/
10MHz

Median nerve



clinicalimage

10/19/2017 14:53:06

q | -
MIQ.73 / TIBD.28

94%

「R」

Preset
MSK
FPS
17
Frequency/
10MHz

Meniscus



3cm

Superficial

HC
HEALCERION
20170208-1

02/08/2017 09:01:40 오전
Healcerion | Unknown
MI:0.00 / TIB:0.00

HC
HEALCERION
20170208-1


02/08/2017 09:17:49 오전
Healcerion | Unknown
MI:0.00 / TIB:0.00

[R]



Preset
Thyroid
FPS
0
Frequency
10 Mhz

[R]

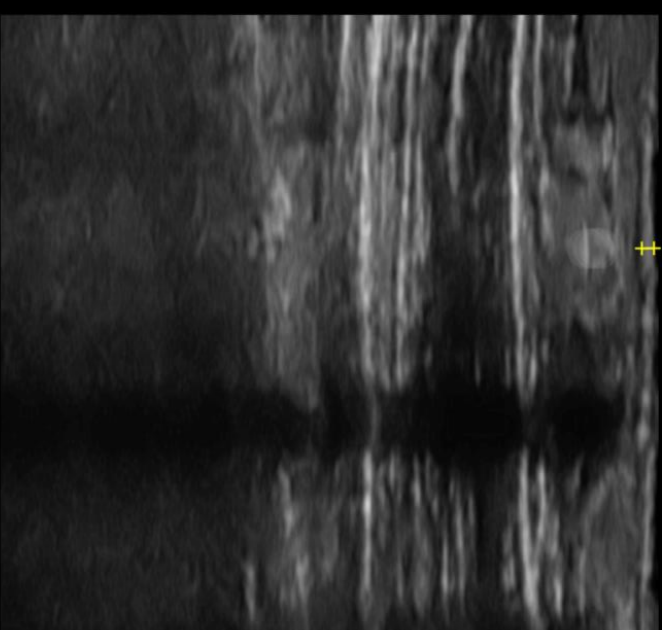

0.7 mm

Preset
Thyroid
FPS
0
Frequency
10 Mhz



Congenital melanocytic nevus

Congenital melanocytic nevus

Dermatology




02/08/2017 10:12:19 오전
Healcerion | Unknown
MI:0.82 / TIB:0.33



02/08/2017 11:01:24 오전
Healcerion | Unknown
MI:0.82 / TIB:0.33

[R]

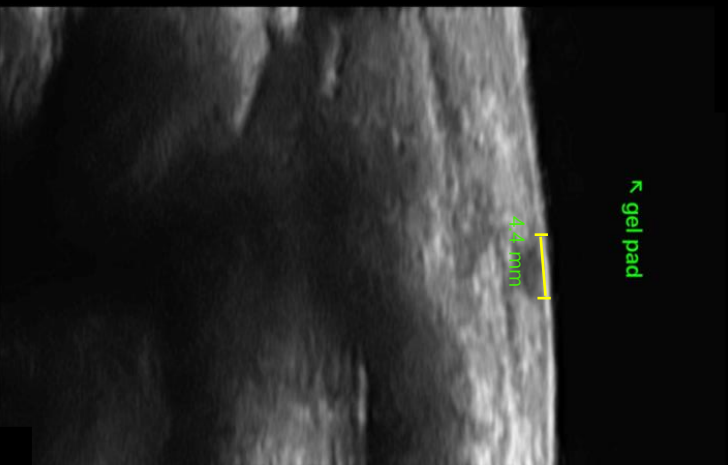

Epidermal cyst

Preset
Thyroid
FPS
0


Frequency
10 Mhz

[R]




Preset
Thyroid
FPS
0

Frequency
10 Mhz

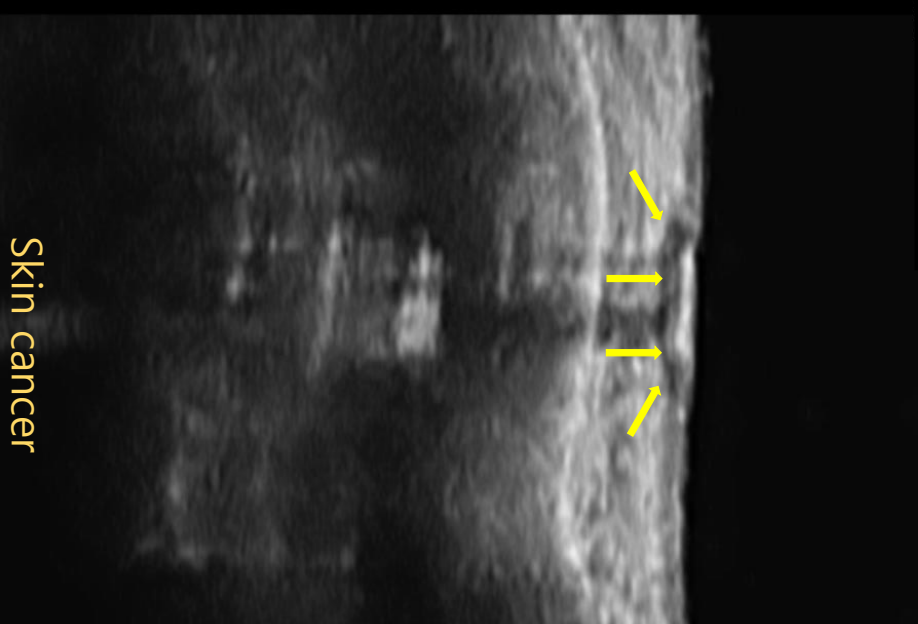


Skin cancer

Aesthetic Procedure

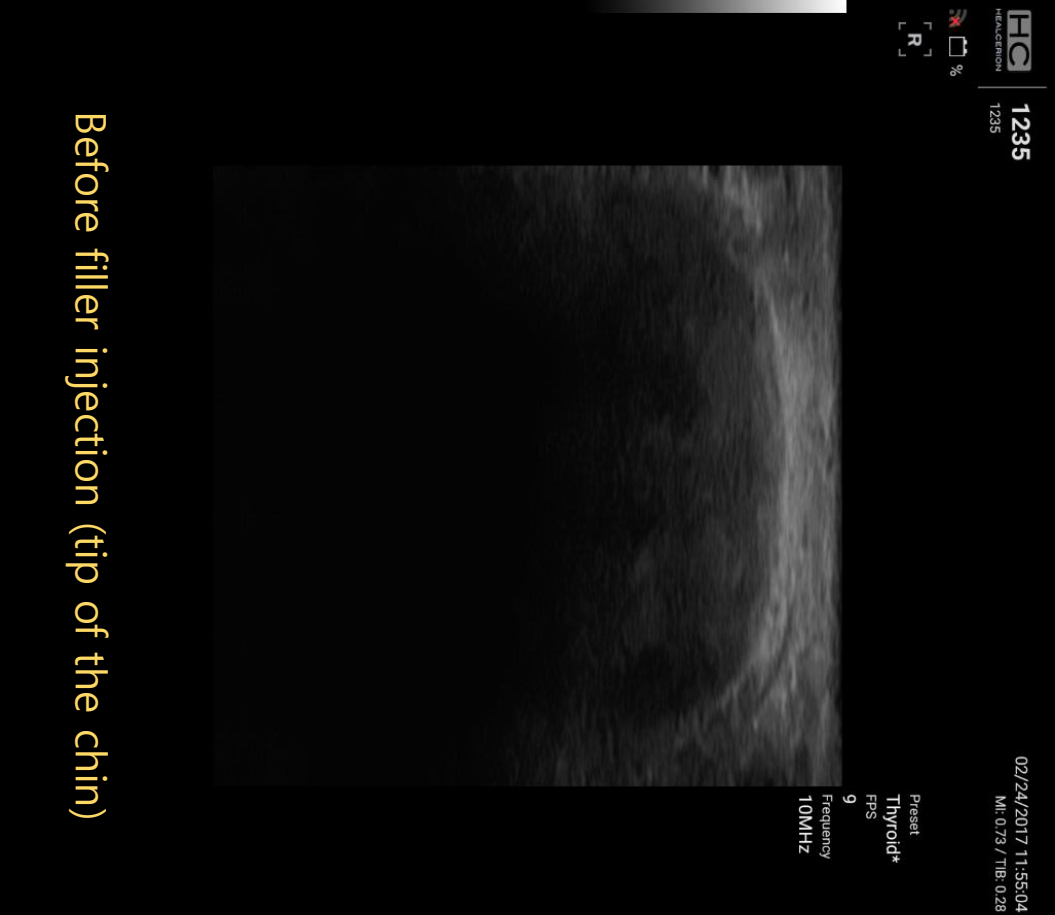


Before filler injection (tip of the chin)

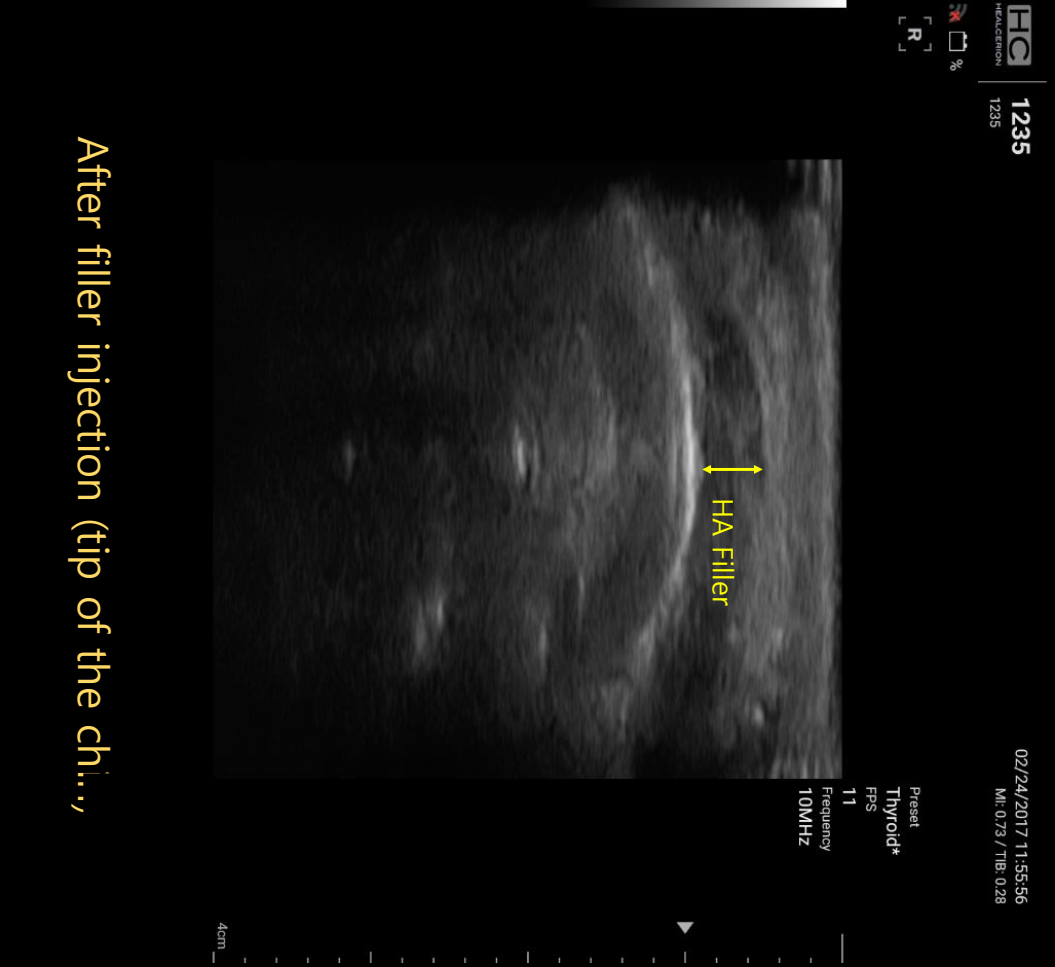


After filler injection (tip of the chin)

Aesthetic Procedure

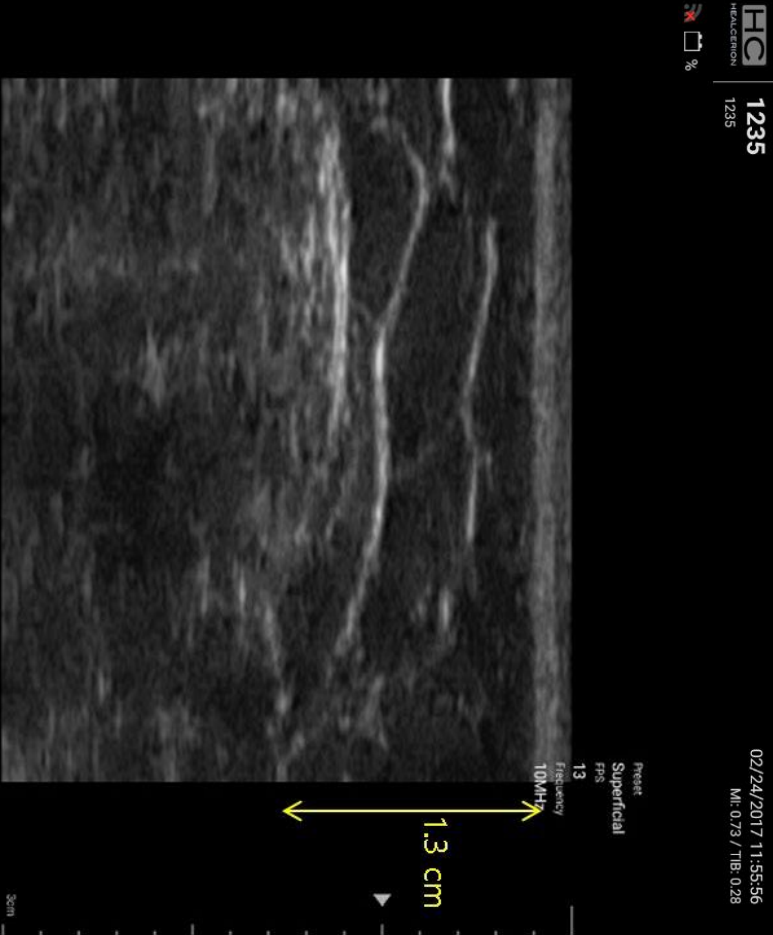

Before liposuction (Rt. Upper arm)

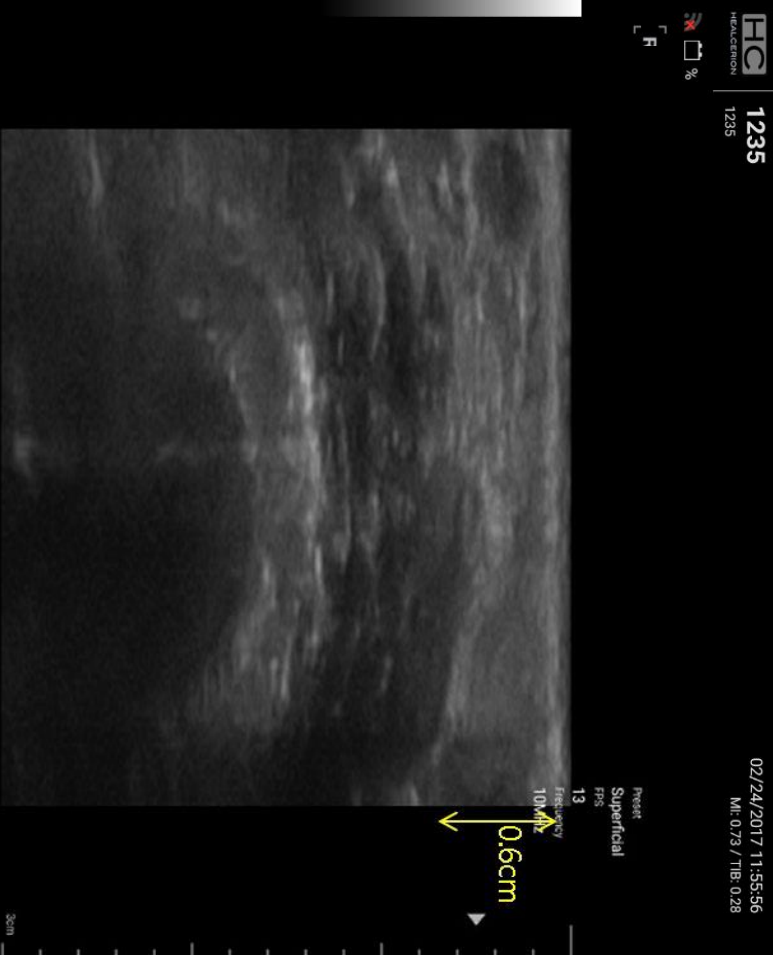

After liposuction (Rt. Upper arm)

Trauma scan

FAST scan



Internal bleeding



Aorta aneurysm


Lung



HEALCERION

20170108

[R]

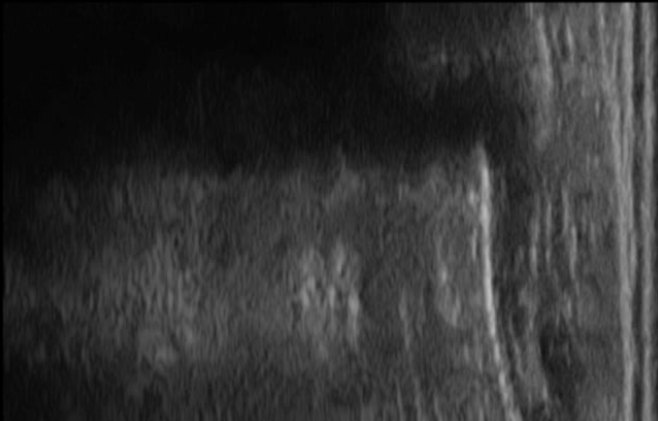

01/09/2017 12:38:41 S21

Healerion | Erika

MI:0.73 / TI:0.28

Preset
Lung

FPS

0



Frequency
10 Mhz



6 cm


Pediatric

Pediatric

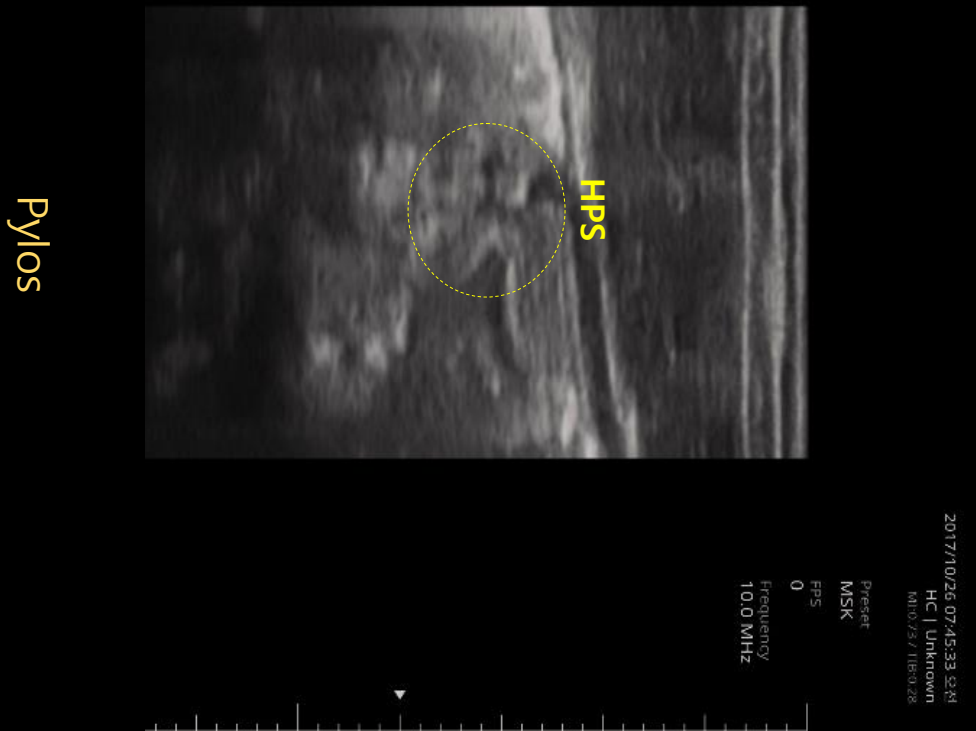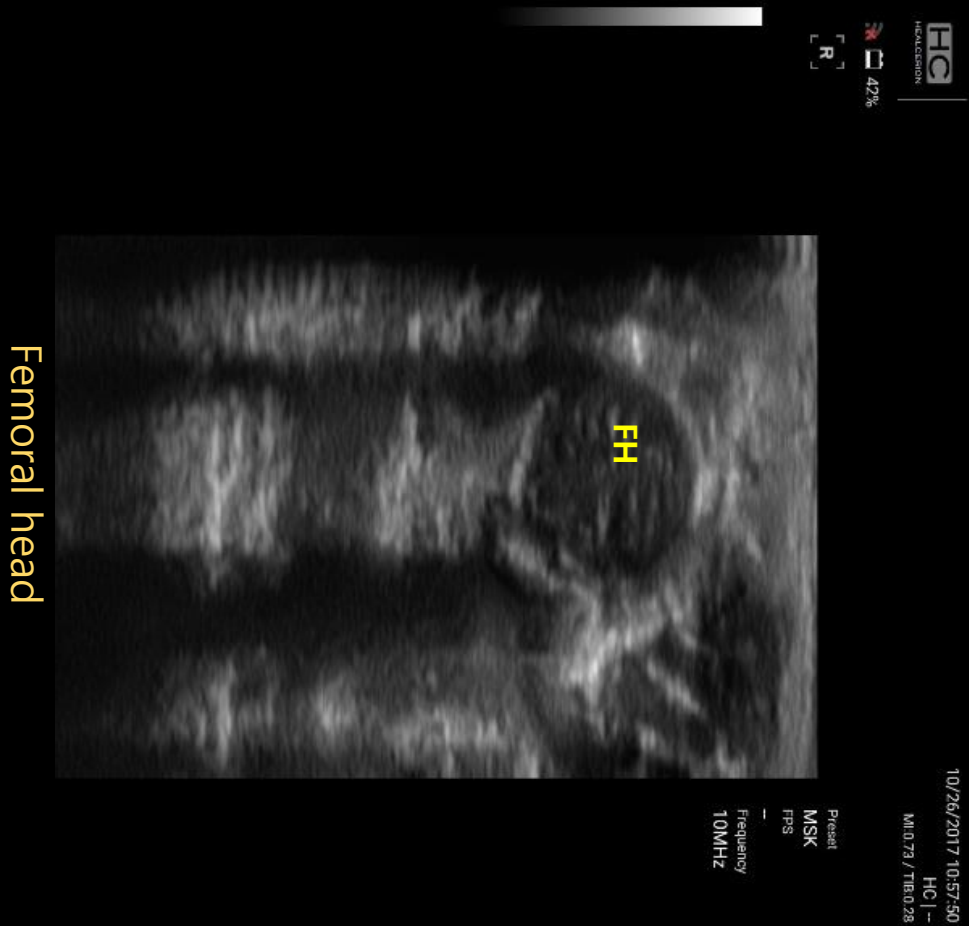

Pediatric

HC
HEALCERION
42%
[R]

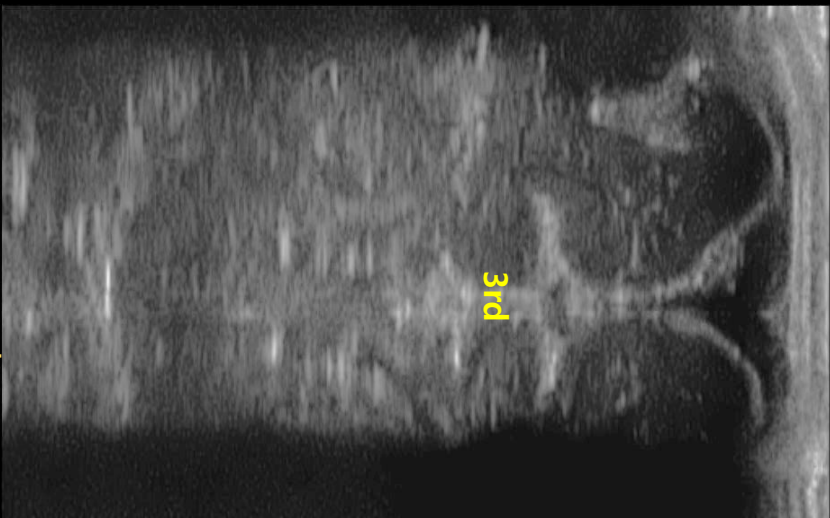


Fontanel

10/24/2017 14:58:09
HC | -
MI:0.73 / TIR:0.28

Preset
FPS
Frequency/
10MHz



HC
HEALCERION
42%
[R]

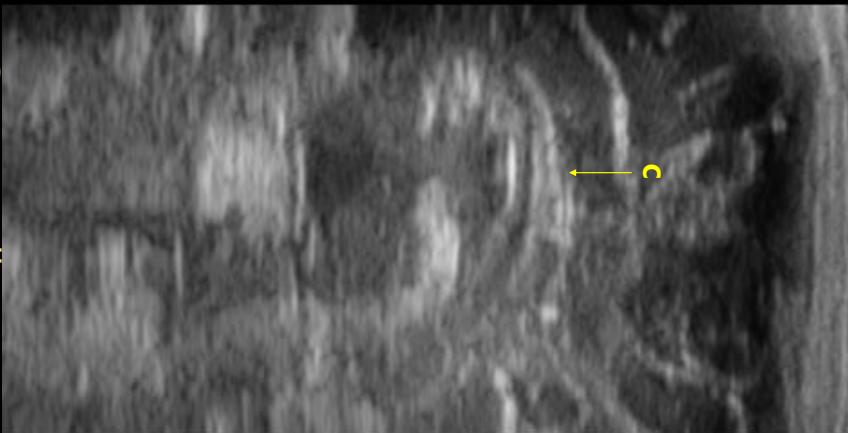

Corpus callosom

10/24/2017 14:58:09
HC | -
MI:0.73 / TIR:0.28


Preset
FPS
Frequency/
10MHz



Pediatric



Post voiding Bladder

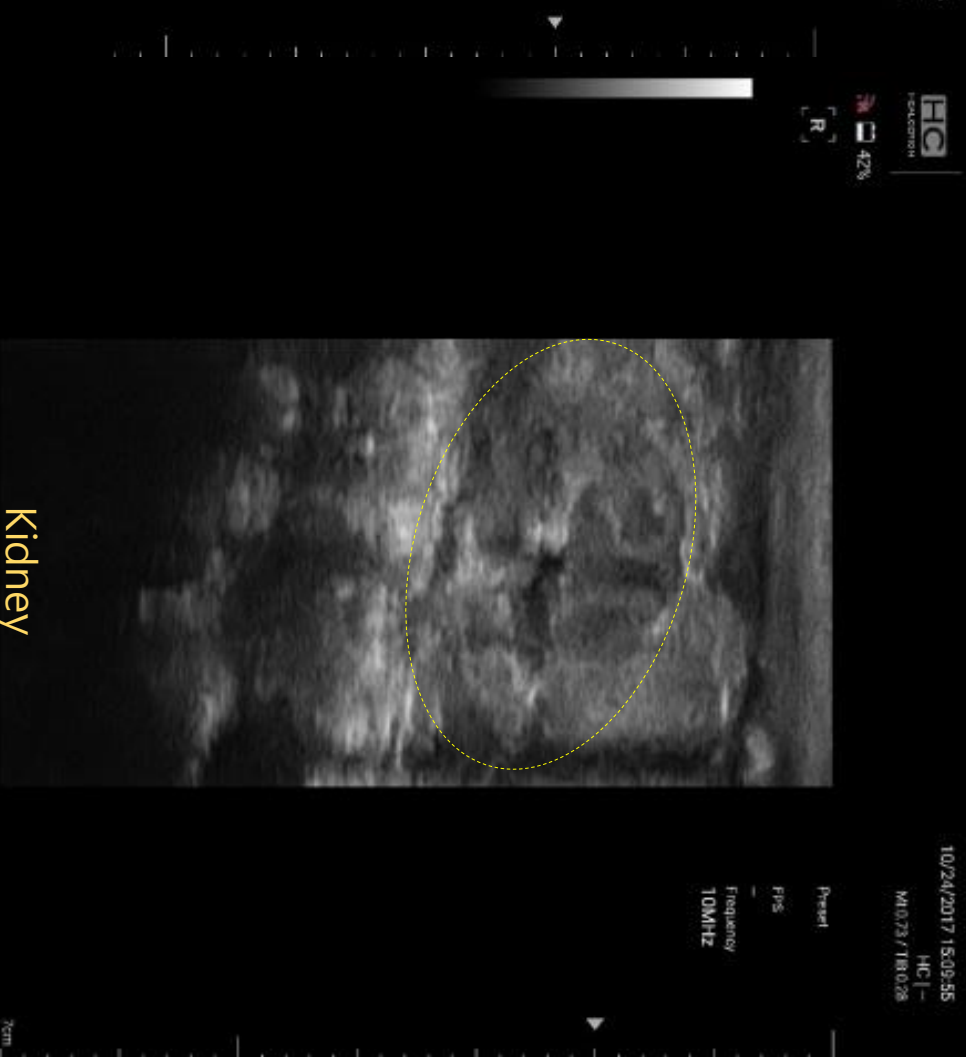

Thank you